

# Model 340 Temperature Controller



## Features

- Operates down to 100 mK with appropriate NTC RTD sensors
- Two sensor inputs; expandable to ten sensor inputs
- Supports diode, RTD, capacitance, and thermocouple sensors
- Sensor excitation current reversal eliminates thermal EMF errors
- Two autotuning control loops: 100 W and 1 W
- IEEE-488 and RS-232C interfaces, analog outputs, digital I/O, and alarm relays

## Product Description

The Model 340 is our most advanced temperature controller and offers unsurpassed resolution, accuracy, and stability for temperature measurement and control applications to as low as 100 mK. Operating with diodes, platinum RTDs, and negative temperature coefficient (NTC) resistor sensors, the Model 340 is expandable to ten sensor inputs or to operate with thermocouple or capacitance sensors. It has two control loops, with the first loop powered to 100 W.

## Sensor Inputs

The Model 340 features two inputs with high-resolution 24-bit analog-to-digital converter and low noise circuit design, providing temperature readings with resolution as low as 0.1 mK at 4.2 K. Sensors are optically isolated from other instrument functions for quiet and repeatable sensor measurements.

Appropriate sensor excitation and input gain can be selected from the front panel. An autorange mode keeps the power in NTC resistors low to reduce self-heating as sensor resistance changes by many orders of magnitude. Automatic current reversal with rounded square wave excitation for NTC resistors eliminates the effect of thermal EMF.

Standard temperature response curves for silicon diodes, platinum RTDs, and many thermocouples are included. Up to twenty 200-point CalCurves™ for Lake Shore calibrated sensors or user curves can be loaded into non-volatile memory via a computer interface or the instrument front panel. CalCurves™ can be installed at the factory when purchased with a Model 340, or they can be field installed using the data card slot. A built-in SoftCal™<sup>1</sup> algorithm can also be used to generate curves for silicon diodes and platinum RTDs, for storage as user curves.

<sup>1</sup> The Lake Shore SoftCal™ algorithm for silicon diode and platinum RTD sensors is a good solution for applications that need more accuracy than a standard sensor curve but do not warrant traditional calibration. SoftCal™ uses the predictability of a standard curve to improve the accuracy of an individual sensor around a few known temperature reference points.

### Temperature Control

The Model 340 offers two proportional-integral-derivative (PID) control loops. A PID control algorithm calculates control output based on temperature setpoint and feedback from the control sensor. Wide tuning parameters accommodate most cryogenic cooling systems and many small high-temperature ovens. Control output is generated by a high-resolution digital-to-analog converter for smooth continuous control. The user can manually set the PID values or the autotuning feature of the Model 340 can automate the tuning process.

The main heater output for the Model 340 is a well-regulated variable DC current source. Heater output is optically isolated from other circuits to reduce interference and ground loops. Heater output can provide up to 100 W of variable DC power to control Loop 1. Features have been added to the Model 340 to minimize the possibility of overheating delicate sensors and wiring in cryostats. These features include setpoint temperature limit, heater current range limit, internal heater diagnostics, and a fuse in the heater output wiring. The Model 340 also has the ability to run a second independent control loop, intended to reduce the temperature gradients in one cooling system rather than to run two different cooling systems.

The setpoint ramp feature allows smooth, continuous changes in setpoint. This feature permits faster experiment cycles, since data can be taken as the system is changing in temperature. It can also be used to make a more predictable approach to a setpoint temperature. The zone feature can automatically change control parameter values for operation over a large temperature range. Values for ten different temperature zones can be loaded into the instrument, which will select the next appropriate zone value on setpoint change.


The Model 340 can run a set of instrument instructions called an internal program. Each program represents the temperature changes needed to conduct a user's experiment. The setpoint can be changed or ramped up and down, and other controller parameters can be programmed. For simple experiments the internal program eliminates the need for computer control. It is also common for the internal program to be used along with the computer interface so the computer is not slowed down by temperature control overhead.

Several math features are included to improve usability and aid in setting up experiments. It is often useful to have reading filters and maximum and minimum calculations easily available on the front panel. The Model 340 also computes a linear equation on reading data to allow flexibility in how the display represents experimental inputs.

### Interface

The Model 340 can be fully involved in computer-controlled experiments. It is equipped with IEEE-488 and RS-232C interfaces. Either interface can send settings to the Model 340 and collect reading data from it. Even the analog outputs, relays, and Digital I/O can be controlled by computer interface.

The Model 340 has several features to make it more valuable as part of a larger measuring system. Two analog voltage outputs can be used to report a voltage that is proportional to the temperature of an input. The outputs can be controlled manually as a voltage source for any other application. Two relays can be used with the alarm setpoints in latching mode for error detection, or in nonlatching mode for simple on and off control. Digital I/O can be used with an external scanner or manually.

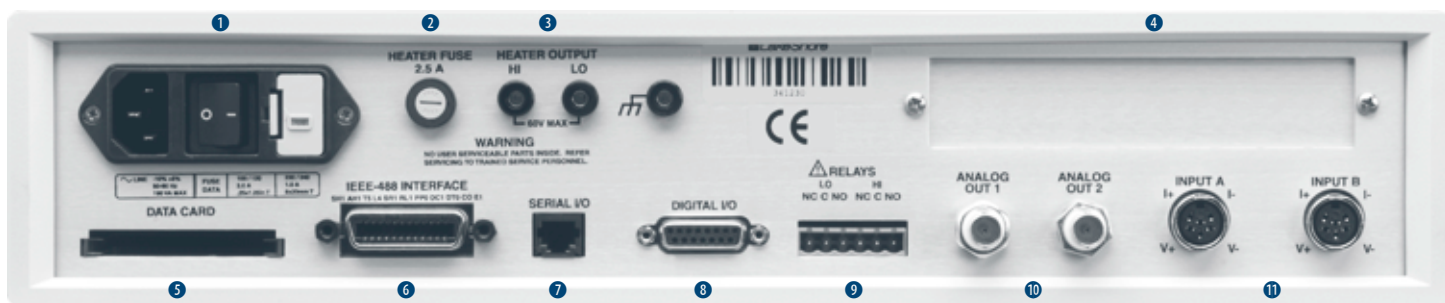


- ❶ - Line Input Assembly
- ❷ - Heater Fuse
- ❸ - Heater Output
- ❹ - Option Slots

- ❺ - Data Card
- ❻ - IEEE-488 Interface
- ❼ - Serial (RS-232C) I/O
- ❽ - Digital I/O


- ❾ - Relays
- ❿ - Analog Outputs
- ⓫ - Standard Sensor Inputs

### Configurable Display


The Model 340 includes a graphic LCD with fluorescent backlight display that is fully configurable and can display up to eight readings.

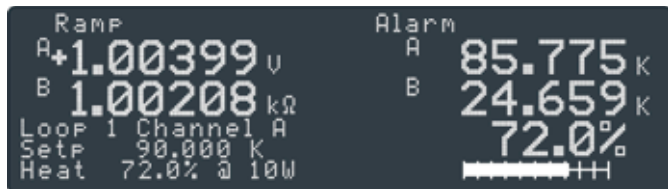

This shows a variation of the display with a large loop 1 heater output graphic bar where the PID parameters are not displayed, but the heater output is more prominent.

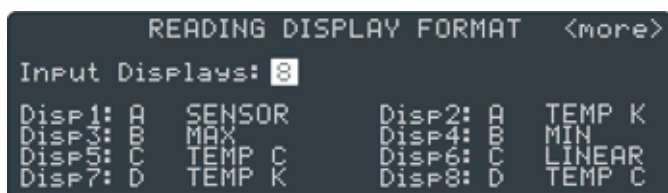

The user can display 1 to 8 readings from any of the available inputs. The units available are the sensor units of mV, V,  $\Omega$ , k $\Omega$ , nF, or temperature units of  $^{\circ}$ C or K. Results of the math feature can also be selected.

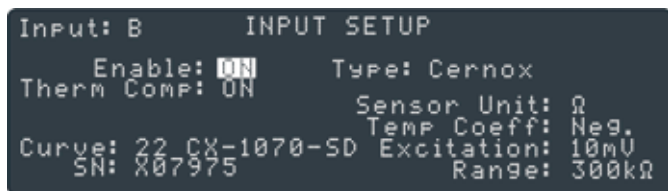

The user can select the sensor type, and the controller will automatically select the sensor units, excitation, and range. If 'special' type is selected, the user can choose any available excitation and input range.

## Additional Inputs Available For Model 340

The following optional inputs are available for the Model 340. Only one can be installed at a time, and the standard inputs stay in the instrument and remain fully functional. Calibration for the option is stored on the card so it can be installed in the field without recalibration.

### 3462 Dual Standard Input Option Card

Adds two standard inputs to the Model 340, appearing on the display as C and D. The card has separate A/Ds and excitation for each sensor. A microprocessor on the card manages the A/D and communication with the Model 340. Allows the Model 340 to read four sensors and use any of them as a control sensor.

### 3464 Dual Thermocouple Input Option Card

Adds two new thermocouple inputs to the Model 340, appearing on the display as C and D. The card has separate A/Ds and excitation for each sensor. A microprocessor on the card manages the A/D and communication with the Model 340. Thermocouple inputs range from cryogenic temperature to 1000  $^{\circ}$ C, with built-in room temperature compensation. Curves for thermocouple types E, K, and AuFe 0.07% vs. Cr are included. The user can add other types.

### 3465 Single Capacitance Input Option Card

Adds a new capacitance input to the Model 340, appearing on the display as C. The card has separate A/D and excitation for the sensor. A microprocessor on the card manages the A/D and communication with the Model 340. The 3465 is intended to control temperature in strong magnetic fields using a Lake Shore Model CS-501 capacitance temperature sensor.

### 3468 Eight Channel Input Option Card

Adds eight sensor inputs to the Model 340. The optional inputs are broken into two groups of four and appear on the display as C1–C4 for Input C, D1–D4 for Input D. The 3468 includes two A/D converters, one for each group of four inputs, and individual excitation for each sensor. Each input group must use the same sensor type, but the two groups can be different. The multiplexed inputs provide new readings for all eight inputs twice each second. The 3468 inputs are not recommended for temperature control because the reading rate is too slow to allow good stability.

A variety of sensor types are supported by the Model 3468, but not as many as the standard inputs. Diode and platinum configurations have similar specifications to the standard inputs, reduced only slightly to account for multiplexing. However, the NTC RTD configuration is quite different than the standard inputs. The option has a limited resistance range of 7.5 k $\Omega$  with a fixed current excitation of 10  $\mu$ A. This limitation significantly reduces the low temperature range of the inputs. The option also does not support current reversal to reduce the effect of thermal EMF voltages. The original standard inputs remain fully functional allowing the Model 340 to measure 10 sensors when the option is installed.

Sensor Temperature Range (sensors sold separately)

		Model	Useful Range	Magnetic Field Use
Diodes 340/3462	Silicon Diode	DT-670-SD	1.4 K to 500 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-670E-BR	30 K to 500 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-414	1.4 K to 375 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-421	1.4 K to 325 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-470-SD	1.4 K to 500 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-471-SD	10 K to 500 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	GaAlAs Diode	TG-120-P	1.4 K to 325 K	$T > 4.2 \text{ K} \ \& \ B \leq 5 \text{ T}$
	GaAlAs Diode	TG-120-PL	1.4 K to 325 K	$T > 4.2 \text{ K} \ \& \ B \leq 5 \text{ T}$
	GaAlAs Diode	TG-120-SD	1.4 K to 500 K	$T > 4.2 \text{ K} \ \& \ B \leq 5 \text{ T}$
Positive Temperature Coefficient RTDs 340/3462	100 $\Omega$ Platinum	PT-102/3	14 K to 873 K	$T > 40 \text{ K} \ \& \ B \leq 2.5 \text{ T}$
	100 $\Omega$ Platinum	PT-111	14 K to 673 K	$T > 40 \text{ K} \ \& \ B \leq 2.5 \text{ T}$
	Rhodium-Iron	RF-800-4	1.4 K to 500 K	$T > 77 \text{ K} \ \& \ B \leq 8 \text{ T}$
	Rhodium-Iron	RF-100T/U	1.4 K to 325 K	$T > 77 \text{ K} \ \& \ B \leq 8 \text{ T}$
Negative Temperature Coefficient RTDs 340/3462	Cernox™	CX-1010	0.3 K to 325 K <sup>3</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Cernox™	CX-1030-HT	0.3 K to 420 K <sup>3,5</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Cernox™	CX-1050-HT	1.4 K to 420 K <sup>3</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Cernox™	CX-1070-HT	4 K to 420 K <sup>3</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Cernox™	CX-1080-HT	20 K to 420 K <sup>3</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Germanium	GR-200A-30	0.1 K to 5 K <sup>5</sup>	Not Recommended
	Germanium	GR-200A-50	0.2 K to 40 K <sup>5</sup>	Not Recommended
	Germanium	GR-200A-100	0.3 K to 100 K	Not Recommended
	Germanium	GR-200A-250	0.5 K to 100 K	Not Recommended
	Germanium	GR-200A/B-500	1.4 K to 100 K	Not Recommended
	Germanium	GR-200A/B-1000	1.4 K to 100 K	Not Recommended
	Germanium	GR-200A/B-1500	1.4 K to 100 K	Not Recommended
	Germanium	GR-200A/B-2500	1.4 K to 100 K	Not Recommended
	Carbon-Glass	CGR-1-500	1.4 K to 325 K	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Carbon-Glass	CGR-1-1000	1.7 K to 325 K <sup>4</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Carbon-Glass	CGR-1-2000	2 K to 325 K <sup>4</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Rox™	RX-102	0.1 K to 40 K <sup>5</sup>	$T > 2 \text{ K} \ \& \ B \leq 10 \text{ T}$
	Rox™	RX-103	1.4 K to 40 K	$T > 2 \text{ K} \ \& \ B \leq 10 \text{ T}$
	Rox™	RX-202	0.1 K to 40 K <sup>5</sup>	$T > 2 \text{ K} \ \& \ B \leq 10 \text{ T}$
Thermocouples 3464	Type K	9006-006	3.2 K to 1505 K	Not Recommended
	Type E	9006-004	3.2 K to 934 K	Not Recommended
	Chromel- AuFe 0.07%	9006-002	1.2 K to 610 K	Not Recommended
Capacitance 3465		CS-501	1.4 K to 290 K	Not Recommended
Diodes 3468	Silicon Diode	DT-670-SD	1.4 K to 500 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-670E-BR	30 K to 500 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-414	1.4 K to 375 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-421	1.4 K to 325 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-470-SD	1.4 K to 500 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	Silicon Diode	DT-471-SD	10 K to 500 K	$T \geq 60 \text{ K} \ \& \ B \leq 3 \text{ T}$
	GaAlAs Diode	TG-120-P	1.4 K to 325 K	$T > 4.2 \text{ K} \ \& \ B \leq 5 \text{ T}$
	GaAlAs Diode	TG-120-PL	1.4 K to 325 K	$T > 4.2 \text{ K} \ \& \ B \leq 5 \text{ T}$
	GaAlAs Diode	TG-120-SD	1.4 K to 500 K	$T > 4.2 \text{ K} \ \& \ B \leq 5 \text{ T}$
Positive Temperature Coefficient RTDs 3468	100 $\Omega$ Platinum	PT-102/3	14 K to 800 K	$T > 40 \text{ K} \ \& \ B \leq 2.5 \text{ T}$
	100 $\Omega$ Platinum	PT-111	14 K to 673 K	$T > 40 \text{ K} \ \& \ B \leq 2.5 \text{ T}$
	Rhodium-Iron	RF-800-4	1.4 K to 500 K	$T > 77 \text{ K} \ \& \ B \leq 8 \text{ T}$
	Rhodium-Iron	RF-100T/U	1.4 K to 325 K	$T > 77 \text{ K} \ \& \ B \leq 8 \text{ T}$
Negative Temperature Coefficient RTDs <sup>2</sup> 3468	Cernox™	CX-1010	2 K to 325 K <sup>5</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Cernox™	CX-1030-HT	3.5 K to 420 K <sup>3,6</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Cernox™	CX-1050-HT	4 K to 420 K <sup>3,6</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Cernox™	CX-1070-HT	15 K to 420 K <sup>3</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Cernox™	CX-1080-HT	50 K to 420 K <sup>3</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Germanium	GR-200A/B-1000	2.2 K to 100 K <sup>4</sup>	Not Recommended
	Germanium	GR-200A/B-1500	2.6 K to 100 K <sup>4</sup>	Not Recommended
	Germanium	GR-200A/B-2500	3.1 K to 100 K <sup>4</sup>	Not Recommended
	Carbon-Glass	CGR-1-500	4 K to 325 K <sup>5</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Carbon-Glass	CGR-1-1000	5 K to 325 K <sup>5</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
	Carbon-Glass	CGR-1-2000	6 K to 325 K <sup>5</sup>	$T > 2 \text{ K} \ \& \ B \leq 19 \text{ T}$
Rox™	RX-102A	1.4 K to 40 K <sup>5</sup>	$T > 2 \text{ K} \ \& \ B \leq 10 \text{ T}$	

**Silicon diodes** are the best choice for general cryogenic use from 1.4 K to above room temperature. Diodes are economical to use because they follow a standard curve and are interchangeable in many applications. They are not suitable for use in ionizing radiation or magnetic fields.

**Cernox™** thin-film RTDs offer high sensitivity and low magnetic field-induced errors over the 0.3 K to 420 K temperature range. Cernox sensors require calibration.

**Platinum RTDs** offer high uniform sensitivity from 30 K to over 800 K. With excellent reproducibility, they are useful as thermometry standards. They follow a standard curve above 70 K and are interchangeable in many applications.

<sup>2</sup> Single excitation current may limit the low temperature range of NTC resistors

<sup>3</sup> Non-HT version maximum temperature: 325 K

<sup>4</sup> Low temperature limited by input resistance range

<sup>5</sup> Low temperature specified with self-heating error:  $\leq 5 \text{ mK}$

<sup>6</sup> Low temperature specified with self-heating error:  $\leq 12 \text{ mK}$

## Sensor Selection

Typical Sensor Performance – see Appendix F for sample calculations of typical sensor performance

	Example Lake Shore Sensor	Temp	Nominal Resistance/ Voltage	Typical Sensor Sensitivity <sup>7</sup>	Measurement Resolution: Temperature Equivalents	Electronic Accuracy: Temperature Equivalents	Temperature Accuracy including Electronic Accuracy, CalCurve™, and Calibrated Sensor	Electronic Control Stability <sup>8</sup> : Temperature Equivalents
<b>340/3462</b>								
<b>Silicon Diode</b>	DT-670-CO-13 with 1.4H calibration	1.4 K	1.664 V	-12.49 mV/K	0.8 mK	±13 mK	±25 mK	±1.6 mK
		77 K	1.028 V	-1.73 mV/K	5.8 mK	±76 mK	±98 mK	±11.6 mK
		300 K	0.5597 V	-2.3 mV/K	4.4 mK	±47 mK	±79 mK	±8.8 mK
		500 K	0.0907 V	-2.12 mV/K	4.8 mK	±40 mK	±90 mK	±9.6 mK
<b>Silicon Diode</b>	DT-470-SD-13 with 1.4H calibration	1.4 K	1.6981 V	-13.1 mV/K	0.8 mK	±13 mK	±25 mK	±1.6 mK
		77 K	1.0203 V	-1.92 mV/K	5.2 mK	±69 mK	±91 mK	±10.4 mK
		300 K	0.5189 V	-2.4 mV/K	4.2 mK	±45 mK	±77 mK	±8.4 mK
		475 K	0.0906 V	-2.22 mV/K	4.5 mK	±38 mK	±88 mK	±9 mK
<b>GaAlAs Diode</b>	TG-120-SD with 1.4H calibration	1.4 K	5.391 V	-97.5 mV/K	0.1 mK	±7 mK	±19 mK	±0.2 mK
		77 K	1.422 V	-1.24 mV/K	8.1 mK	±180 mK	±202 mK	±16.2 mK
		300 K	0.8978 V	-2.85 mV/K	3.6 mK	±60 mK	±92 mK	±7.2 mK
		475 K	0.3778 V	-3.15 mV/K	3.2 mK	±38 mK	±88 mK	±6.4 mK
<b>100 Ω Platinum RTD 500 Ω Full Scale</b>	PT-103 with 14J calibration	30 K	3.660 Ω	0.191 Ω/K	5.3 mK	±13 mK	±23 mK	±10.6 mK
		77 K	20.38 Ω	0.423 Ω/K	2.4 mK	±10 mK	±22 mK	±4.8 mK
		300 K	110.35 Ω	0.387 Ω/K	2.6 mK	±34 mK	±57 mK	±5.2 mK
		500 K	185.668 Ω	0.378 Ω/K	2.7 mK	±55 mK	±101 mK	±5.4 mK
<b>Cernox™</b>	CX-1010-SD with 0.3L calibration	0.3 K	2322.4 Ω	-10785 Ω/K	3 μK	±0.2 mK	±3.7 mK	±6 μK
		0.5 K	1248.2 Ω	-2665.2 Ω/K	12 μK	±0.5 mK	±5 mK	±24 μK
		4.2 K	277.32 Ω	-32.209 Ω/K	94 μK	±6.2 mK	±11.2 mK	±188 μK
		300 K	30.392 Ω	-0.0654 Ω/K	15 mK	±540 mK	±580 mK	±30 mK
<b>Cernox™</b>	CX-1050-SD-HT <sup>9</sup> with 1.4M calibration	1.4 K	26566 Ω	-48449 kΩ/K	6 μK	±0.4 mK	±5.4 mK	±12 μK
		4.2 K	3507.2 Ω	-1120.8 kΩ/K	90 μK	±3.4 mK	±8.4 mK	±180 μK
		77 K	205.67 Ω	-2.4116 Ω/K	1.3 mK	±68 mK	±84 mK	±2.6 mK
		420 K	45.03 Ω	-0.0829 Ω/K	12 mK	±520 mK	±585 mK	±24 mK
<b>Germanium</b>	GR-200A-250 with 0.5D calibration	0.5 K	29570 Ω	-221000 Ω/K	14 μK	±0.2 mK	±4.5 mK	±28 μK
		1.4 K	1376 Ω	-2220 Ω/K	140 μK	±0.9 mK	±4.9 mK	±280 μK
		4.2 K	198.9 Ω	-68.9 Ω/K	440 μK	±3.8 mK	±7.8 mK	±880 μK
		100 K	2.969 Ω	-0.025 Ω/K	40 mK	±200 mK	±216 mK	±80 mK
<b>Germanium</b>	GR-200A-500 with 0.5D calibration	1.4 K	8257 Ω	-19400 kΩ/K	52 μK	±0.6 mK	±4.6 mK	±104 μK
		4.2 K	520 Ω	-245 kΩ/K	410 μK	±3.0 mK	±7 mK	±820 μK
		10 K	88.41 Ω	-19.5 Ω/K	515 μK	±5.6 mK	±10.6 mK	±1.03 mK
		100 K	1.751 Ω	-0.014 Ω/K	72 mK	±270 mK	±286 mK	±114 mK
<b>Carbon-Glass</b>	CGR-1-500 with 1.4L calibration	1.4 K	103900 Ω	-520000 Ω/K	58 μK	±0.6 mK	±4.6 mK	±116 μK
		4.2 K	584.6 Ω	-422.3 Ω/K	24 μK	±1.2 mK	±5.2 mK	±48 μK
		77 K	14.33 Ω	-0.098 Ω/K	3.1 mK	±140 mK	±165 mK	±6.2 mK
		300 K	8.55 Ω	-0.0094 Ω/K	32 mK	±1.1 K	±1.2 K	±64 mK
<b>Rox™</b>	RX-102A-AA with 0.3B calibration	0.5 K	3701 Ω	-5478 Ω/K	19 μK	±0.7 mK	±5.2 mK	±38 μK
		1.4 K	2005 Ω	-667 Ω/K	45 μK	±2.4 mK	±7.4 mK	±90 μK
		4.2 K	1370 Ω	-80.3 Ω/K	375 μK	±16 mK	±32 mK	±750 μK
		40 K	1049 Ω	-1.06 Ω/K	29 mK	±1.1 K	±1.2 K	±58 mK
<b>Thermocouple 50 mV 3464</b>	Type K	75 K	-5862.9 μV	15.6 μV/K	26 mK	±0.124 K	Calibration not available from Lake Shore	±52 mK
		300 K	1075.3 μV	40.6 μV/K	10 mK	±0.038 K		±20 mK
		600 K	13325 μV	41.7 μV/K	10 mK	±0.184 K		±20 mK
		1505 K	49998.3 μV	36.006 μV/K	12 mK	±0.73 K		±24 mK
<b>Capacitance 150 nF 3465</b>	CS-501GR	4.2 K	6 nF	27 pF/K	7.4 mK	±2.08 K	Calibration not available from Lake Shore	±14.8 mK
		77 K	9.1 nF	52 pF/K	3.9 mK	±1.14 K		±7.8 mK
		200 K	19.2 nF	174 pF/K	1 mK	±0.4 K		±2 mK

<sup>7</sup> Typical sensor sensitivities were taken from representative calibrations for the sensor listed

<sup>8</sup> Control stability of the electronics only, in an ideal thermal system

<sup>9</sup> Non-HT version maximum temperature: 325 K

# Specifications

## Input Specifications

	Sensor Temperature Coefficient	Input Range	Excitation Current	Display Resolution	Measurement Resolution	Electronic Accuracy	Electronic Control Stability <sup>10</sup>
<b>Diode</b> 340/3462	negative	0 V to 2.5 V	10 $\mu$ A $\pm$ 0.05%	10 $\mu$ V	10 $\mu$ V	$\pm$ 80 $\mu$ V $\pm$ 0.005% of rdg	20 $\mu$ V
	negative	0 V to 7.5 V	10 $\mu$ A $\pm$ 0.05%	10 $\mu$ V	10 $\mu$ V	$\pm$ 80 $\mu$ V $\pm$ 0.01% of rdg	20 $\mu$ V
<b>PTC RTD</b> 340/3462	positive	0 $\Omega$ to 250 $\Omega$	1 mA	1 m $\Omega$	1 m $\Omega$	$\pm$ 0.002 $\Omega$ $\pm$ 0.01% of rdg	2 m $\Omega$
	positive	0 $\Omega$ to 500 $\Omega$	1 mA	1 m $\Omega$	1 m $\Omega$	$\pm$ 0.002 $\Omega$ $\pm$ 0.01% of rdg	2 m $\Omega$
	positive	0 $\Omega$ to 2500 $\Omega$	0.1 mA	10 m $\Omega$	10 m $\Omega$	$\pm$ 0.03 $\Omega$ $\pm$ 0.02% of rdg	20 m $\Omega$
<b>NTC RTD</b> 1 mV 340/3462	negative	0 $\Omega$ to 10 $\Omega$	100 $\mu$ A	100 $\mu$ $\Omega$	1 m $\Omega$	$\pm$ 0.02% rng $\pm$ 0.1% rdg	2 m $\Omega$
	negative	0 $\Omega$ to 30 $\Omega$	30 $\mu$ A	100 $\mu$ $\Omega$	3 m $\Omega$	$\pm$ 0.02% rng $\pm$ 0.1% rdg	6 m $\Omega$
	negative	0 $\Omega$ to 100 $\Omega$	10 $\mu$ A	1 m $\Omega$	10 m $\Omega$	$\pm$ 0.02% rng $\pm$ 0.1% rdg	20 m $\Omega$
	negative	0 $\Omega$ to 300 $\Omega$	3 $\mu$ A	1 m $\Omega$	30 m $\Omega$	$\pm$ 0.02% rng $\pm$ 0.1% rdg	60 m $\Omega$
	negative	0 $\Omega$ to 1 k $\Omega$	1 $\mu$ A	10 m $\Omega$	0.1 $\Omega$	$\pm$ 0.02% rng $\pm$ 0.1% rdg	0.2 $\Omega$
	negative	0 $\Omega$ to 3 k $\Omega$	300 nA	10 m $\Omega$	0.3 $\Omega$	$\pm$ 0.02% rng $\pm$ 0.1% rdg	0.6 $\Omega$
	negative	0 $\Omega$ to 10 k $\Omega$	100 nA	0.1 $\Omega$	1 $\Omega$	$\pm$ 0.02% rng $\pm$ 0.1% rdg	2 $\Omega$
	negative	0 $\Omega$ to 30 k $\Omega$	30 nA	0.1 $\Omega$	3 $\Omega$	$\pm$ 0.02% rng $\pm$ 0.1% rdg	6 $\Omega$
<b>NTC RTD</b> 10 mV 340/3462	negative	0 $\Omega$ to 30 $\Omega$	300 $\mu$ A	100 $\mu$ $\Omega$	300 $\mu$ $\Omega$	$\pm$ 0.02% rng $\pm$ 0.05% rdg	600 $\mu$ $\Omega$
	negative	0 $\Omega$ to 100 $\Omega$	100 $\mu$ A	1 m $\Omega$	1 m $\Omega$	$\pm$ 0.02% rng $\pm$ 0.05% rdg	2 m $\Omega$
	negative	0 $\Omega$ to 300 $\Omega$	30 $\mu$ A	1 m $\Omega$	3 m $\Omega$	$\pm$ 0.02% rng $\pm$ 0.05% rdg	6 m $\Omega$
	negative	0 $\Omega$ to 1 k $\Omega$	10 $\mu$ A	10 m $\Omega$	10 m $\Omega$	$\pm$ 0.02% rng $\pm$ 0.05% rdg	20 m $\Omega$
	negative	0 $\Omega$ to 3 k $\Omega$	3 $\mu$ A	10 m $\Omega$	30 m $\Omega$	$\pm$ 0.02% rng $\pm$ 0.05% rdg	60 m $\Omega$
	negative	0 $\Omega$ to 10 k $\Omega$	1 $\mu$ A	0.1 $\Omega$	0.1 $\Omega$	$\pm$ 0.02% rng $\pm$ 0.05% rdg	0.2 $\Omega$
	negative	0 $\Omega$ to 30 k $\Omega$	300 nA	0.1 $\Omega$	0.3 $\Omega$	$\pm$ 0.02% rng $\pm$ 0.05% rdg	0.6 $\Omega$
	negative	0 $\Omega$ to 100 k $\Omega$	100 nA	1 $\Omega$	3 $\Omega$	$\pm$ 0.02% rng $\pm$ 0.05% rdg	6 $\Omega$
<b>Thermocouple</b> 3464	positive	$\pm$ 25 mV	NA	0.1 $\mu$ V	0.2 $\mu$ V	$\pm$ 1 $\mu$ V $\pm$ 0.05% of rdg	0.4 $\mu$ V
	positive	$\pm$ 50 mV	NA	0.1 $\mu$ V	0.4 $\mu$ V	$\pm$ 1 $\mu$ V $\pm$ 0.05% of rdg	0.8 $\mu$ V
<b>Capacitance</b> 3465	positive or negative	0 nF to 150 nF	4.88 kHz 1 V square wave	10 pF	2.0 pF	$\pm$ 50 pF $\pm$ 0.1% of rdg	4.0 pF
	positive or negative	0 nF to 15 nF	4.88 kHz 1 V square wave	1 pF	0.2 pF	$\pm$ 50 pF $\pm$ 0.1% of rdg	0.4 pF
<b>Diode</b> 3468	negative	0 V to 2.5 V	10 $\mu$ A $\pm$ 0.01%	100 $\mu$ V	20 $\mu$ V	$\pm$ 160 $\mu$ V $\pm$ 0.01% of rdg	40 $\mu$ V
	negative	0 V to 7.5 V	10 $\mu$ A $\pm$ 0.01%	100 $\mu$ V	20 $\mu$ V	$\pm$ 160 $\mu$ V $\pm$ 0.02% of rdg	40 $\mu$ V
<b>PTC RTD</b> 3468	positive	0 $\Omega$ to 250 $\Omega$	1 mA $\pm$ 0.3%	10 m $\Omega$	2 m $\Omega$	$\pm$ 0.004 $\Omega$ $\pm$ 0.02% of rdg	4 m $\Omega$
	positive	0 $\Omega$ to 500 $\Omega$	1 mA $\pm$ 0.3%	10 m $\Omega$	2 m $\Omega$	$\pm$ 0.004 $\Omega$ $\pm$ 0.02% of rdg	4 m $\Omega$
	positive	0 $\Omega$ to 5000 $\Omega$	1 mA $\pm$ 0.3%	100 m $\Omega$	20 m $\Omega$	$\pm$ 0.06 $\Omega$ $\pm$ 0.04% of rdg	40 m $\Omega$
<b>NTC RTD</b> 3468	negative	0 $\Omega$ to 7500 $\Omega$	10 $\mu$ A $\pm$ 0.01%	100 m $\Omega$	50 m $\Omega$	$\pm$ 0.01 $\Omega$ $\pm$ 0.04% of rdg	0.1 $\Omega$

<sup>10</sup> Control stability of the electronics only, in an ideal thermal system

### Thermometry

- Number of inputs** 2 included (additional inputs optional)
- Input configuration** Each input is factory configured as diode/RTD. Thermocouple and capacitance are optional and sold as additional input cards.
- Isolation** Sensor inputs optically isolated from other circuits but not from each other
- A/D resolution** 24-bit analog-to-digital
- Input accuracy** Sensor dependent – refer to Input Specifications table
- Measurement resolution** Sensor dependent – refer to Input Specifications table
- Maximum update rate** Up to 20 readings per s on an input, 40 readings per s on all inputs
- Autorange** Automatically selects appropriate NTC RTD range
- User curves** Forty 200-point CalCurves™, or user curves
- SoftCal™** Improves accuracy of DT-470 diode or platinum RTD sensors
- Math** Maximum and minimum of input readings and linear equation
- Filter** Averages input readings to quiet display, settable time constant

### Sensor Input Configuration

	Diode/RTD	Thermocouple	Capacitance
<b>Measurement type</b>	4-lead differential	2-lead, room temperature compensated	4-lead
<b>Excitation</b>	Constant current with current reversal for RTDs	NA	4.88 kHz, 1 V square wave
<b>Supported sensors</b>	Diodes: Silicon, GaAlAs RTDs: 100 $\Omega$ Platinum, 1000 $\Omega$ Platinum, Germanium, Carbon-Glass, Cernox™, and Rox™	Most thermocouple types	CS-501GR
<b>Standard curves</b>	DT-470, DT-500D, DT-670, PT-100, PT-1000, RX-102A, RX-202A	Type E, Type K, Type T AuFe 0.07% vs. Cr, AuFe 0.03% vs. Cr,	None
<b>Input connector</b>	6-pin DIN	Ceramic isothermal block	6-pin DIN

**Control**

<b>Control loops</b>	2
<b>Control type</b>	Closed-loop digital PID with manual heater power output, or open loop
<b>Tuning</b>	Autotune (one loop at a time), manual PID, zones
<b>Control stability</b>	Sensor dependent – to 2× measurement resolution (in an ideal thermal system)
<b>PID control settings</b>	
<b>Proportional (gain)</b>	0 to 1000 with 0.1 setting resolution
<b>Integral (reset)</b>	1 to 1000 with 0.1 setting resolution
<b>Derivative (rate)</b>	1 to 1000 s with 1 s resolution
<b>Manual output</b>	0 to 100% with 0.01% setting resolution
<b>Zone control</b>	10 temperature zones with P, I, D, manual heater power out, and heater range
<b>Setpoint ramping</b>	0.1 K per min to 100 K per min
<b>Safety limits</b>	Setpoint limit, curve temp limits, heater output, slope limit, heater range limit, power up heater off, and short-circuit protection

**Heater Output Specifications**

	Loop 1	Loop 2
<b>Heater output type</b>	Variable DC current source	Variable DC voltage
<b>Heater output D/A resolution</b>	18-bit	14-bit
<b>Max heater power</b>	100 W	1 W
<b>Max heater output current</b>	2 A	0.1 A
<b>Heater output compliance</b>	50 V	10 V
<b>Heater source impedance</b>	NA	0.01 Ω
<b>Heater output ranges</b>	5 decade steps in power	1
<b>Heater load type</b>	Resistive	Resistive
<b>Heater load range</b>	10 Ω to 100 Ω recommended	100 Ω minimum
<b>Heater load for max power</b>	25 Ω	100 Ω
<b>Heater noise (&lt;1 kHz) RMS</b>	50 μV + 0.001% of output voltage	<0.3 mV
<b>Isolation</b>	Optical isolation between output and other circuits	None
<b>Heater connector</b>	Dual banana	BNC

**Loop 1 Full Scale Heater Power at Typical Resistance**

Heater Resistance	Heater Range	Maximum Current			
		2 A	1 A	0.5 A	0.25 A
10 Ω	5	40 W	10 W	2.5 W	625 mW
	4	4 W	1 W	250 mW	62.5 mW
	3	0.4 W	100 mW	25 mW	6.25 mW
	2	40 mW	10 mW	2.5 mW	625 μW
	1	4 mW	1 mW	250 μW	62.5 μW
25 Ω	5	100 W	25 W	6.25 W	1.56 W
	4	10 W	2.5 W	625 mW	156 mW
	3	1 W	250 mW	62.5 mW	15.6 mW
	2	100 mW	25 mW	6.25 mW	1.56 mW
	1	10 mW	2.5 mW	625 μW	156 μW
50 Ω	5	50 W	50 W	12.5 W	3.12 W
	4	20 W	5 W	1.25 W	312 mW
	3	2 W	500 mW	125 mW	31.2 mW
	2	200 mW	50 mW	12.5 mW	3.12 mW
	1	20 mW	5 mW	1.25 mW	312 μW

**Front Panel**


<b>Display</b>	Graphic LCD with fluorescent backlight
<b>No. of reading displays</b>	1 to 8
<b>Display units</b>	Temperature in K, °C, or sensor units
<b>Temp display resolution</b>	0.0001 K below 10 K, 0.001 K above 10 K
<b>Sensor units display resolution</b>	Sensor dependent, to 6 digits
<b>Setpoint setting resolution</b>	Same as display resolution (actual resolution is sensor dependent)
<b>Heater output display</b>	Numeric display in percent of full scale for power or current – bar graph display of heater output available
<b>Heater output resolution</b>	0.1% numeric or 2% graphical
<b>Keypad</b>	Numeric plus special function
<b>Front panel features</b>	Front panel curve entry, display brightness control, and keypad lock-out

**Interfaces**

<b>IEEE-488.2 interface</b>	
<b>Features</b>	SH1, AH1, T5, L4, SR1, RL1, PP0, DC1, DT0, C0, E1
<b>Reading rate</b>	To 20 readings per s
<b>Software support</b>	National Instruments LabVIEW™ driver
<b>Serial interface</b>	
<b>Electrical format</b>	RS-232C
<b>Max baud rate</b>	19,200 baud
<b>Connector</b>	RJ-11
<b>Reading rate</b>	To 20 readings per s
<b>Alarms</b>	
<b>Number</b>	Two, high and low, for each installed input
<b>Data source</b>	Temperature, Sensor Units, and Linear Equation
<b>Settings</b>	Source, High and Low Setpoint, Latching or Non-Latching, and Audible On/Off
<b>Actuators</b>	Display, annunciator, beeper, and relays
<b>Relays</b>	
<b>Number</b>	2
<b>Contacts</b>	Normally open (NO), normally closed (NC), and common
<b>Contact Rating</b>	30 VDC at 2 A
<b>Operation</b>	Activate relays on high or low alarms for any input, or manual off/on
<b>Connector</b>	Detachable terminal block
<b>Analog voltage outputs</b> (when not used as control loop 2 output)	
<b>Number</b>	2
<b>Scale</b>	User selected
<b>Update rate</b>	20 readings per s
<b>Data source</b>	Temperature, Sensor Units, and Linear Equation
<b>Settings</b>	Input, Source, Top of Scale, Bottom of Scale, or Manual
<b>Range</b>	±10 V
<b>Resolution</b>	1.25 mV
<b>Max output power</b>	1 W
<b>Min load resistance</b>	100 Ω (short-circuit protected)
<b>Source impedance</b>	0.01 Ω
<b>Digital I/O</b>	5 inputs and 5 outputs – TTL voltage level compatible
<b>Data card</b>	PC card Type II slot used for curve transfer, setup storage, and data-logging
<b>General</b>	
<b>Ambient temp range</b>	20 °C to 30 °C (68 °F to 86 °F) for specified accuracy; 15 °C to 35 °C (59 °F to 95 °F) for reduced accuracy
<b>Power requirements</b>	100, 120, 220, 240 VAC (+5%, -10%), 50 or 60 Hz; 190 VA
<b>Size</b>	432 mm W × 89 mm H × 368 mm D (17 in × 3.5 in × 14.5 in), full rack
<b>Weight</b>	8 kg (17.6 lb) approx.
<b>Approval</b>	CE mark

**Extending Temperature Controller Heater Power**

It is often necessary to extend the heater power of a cryogenic temperature controller to conduct experiments above room temperature. This diagram illustrates a practical way to increase the control output of the Model 340 to several hundred watts. A programming resistor,  $R_{pgm}$ , is placed across the controller's heater output current source. As the heater output current changes, a changing voltage is generated across  $R_{pgm}$ . That voltage is used to program a large external power supply.  $R_{pgm}$  should be chosen so that a low current range of the controller can be used. The control output of loop 2 on the Model 340 is a voltage, thus it can be connected directly to the external power supply without  $R_{pgm}$ .

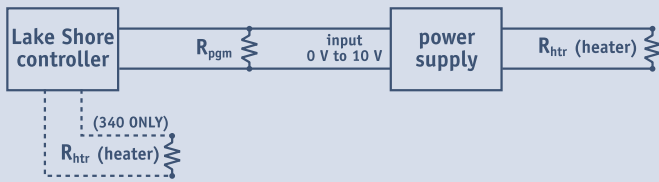

**3003 Heater Output Conditioner**

The heater output conditioner is a passive filter which further reduces the already low Model 340 heater output noise. The typical insertion loss for the Model 3003 is 20 dB at or above line frequency, and >40 dB at or above double line frequency. A 144 mm W x 72 mm H x 165 mm D (5.7 in x 2.8 in x 6.5 in) panel mount enclosure houses this option, and it weighs 1.6 kg (3.5 lb).



**Ordering Information**

Part number	Description
<b>340</b>	2 diode/resistor inputs temperature controller
<b>Select a power configuration*:</b>	
<b>VAC-100</b>	Instrument configured for 100 VAC with U.S. power cord
<b>VAC-120</b>	Instrument configured for 120 VAC with U.S. power cord
<b>VAC-120-ALL</b>	Instrument configured for 120 VAC with U.S. power cord and universal Euro line cord and fuses for 220/240 VAC setting
<b>VAC-220</b>	Instrument configured for 220 VAC with universal Euro line cord
<b>VAC-240</b>	Instrument configured for 240 VAC with universal Euro line cord
<i>*Other country line cords available, consult Lake Shore</i>	
<b>Accessories included</b>	
<b>106-009</b>	Heater output connector (dual banana jack)
<b>106-233</b>	Two sensor mating connector 6-pin DIN plugs used for sensor inputs
<b>106-737</b>	6-pin terminal block used for relays connector – accepts up to 12 AWG wire
<b>2001</b>	4-wire RJ11 cable assembly, 4.6 m (14 ft) long, used with RS-232C interface
<b>2003</b>	RJ11 to DE-9 adapter – adapts RJ11 receptacle to female DE-9 connector; connects Model 340 to customer computer rear RS-232C serial port
	Calibration certificate
<b>MAN-340</b>	Model 340 user manual
<b>Options and accessories</b>	
<b>2002</b>	RJ11 to DB-25 adapter
<b>2003</b>	RJ11 to DE-9 adapter
<b>3003</b>	Heater output conditioner
<b>3462</b>	2-channel card for additional standard sensors
<b>3464</b>	2-channel card for thermocouple sensors
<b>3465</b>	1-channel card for capacitance sensors
<b>3468</b>	8-channel scanner card for silicon diodes, PTC and NTC RTD sensors
<b>3507-2SH</b>	Cable assembly for 2 sensors and 1 heater
<b>8001-340</b>	CalCurve™, factory installed – the breakpoint table from a calibrated sensor stored in the instrument
<b>8072</b>	IEEE-488 computer interface interconnect cable assembly
<b>CAL-340-CERT</b>	Instrument calibration with certificate
<b>HTR-25</b>	25 Ω, 25 W cartridge heater
<b>HTR-50</b>	50 Ω, 50 W cartridge heater
<b>RM-1</b>	Rack mounting kit

